


HPLC DATA SHEET

β-Carotene

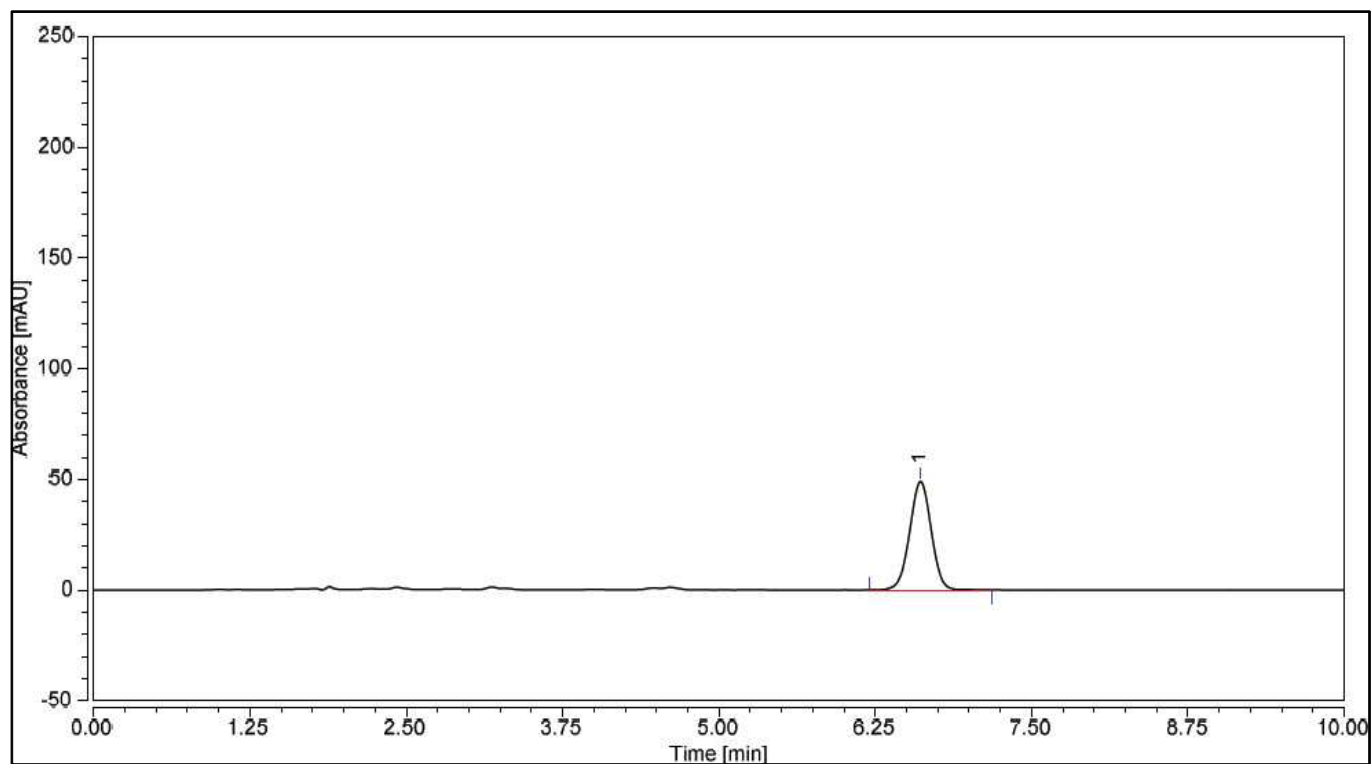

1. β-carotene

HPLC condition

Column	INNO Column C18 (5μm, 4.6mm I.d. × 150mm)
Mobile Phase	TFA / Ethanol = 1 / 99
Flow rate	1.0 mL/min
Temperature	35℃
Detector	UV (450nm)