


HPLC DATA SHEET

Bosentan (USP, Assay)

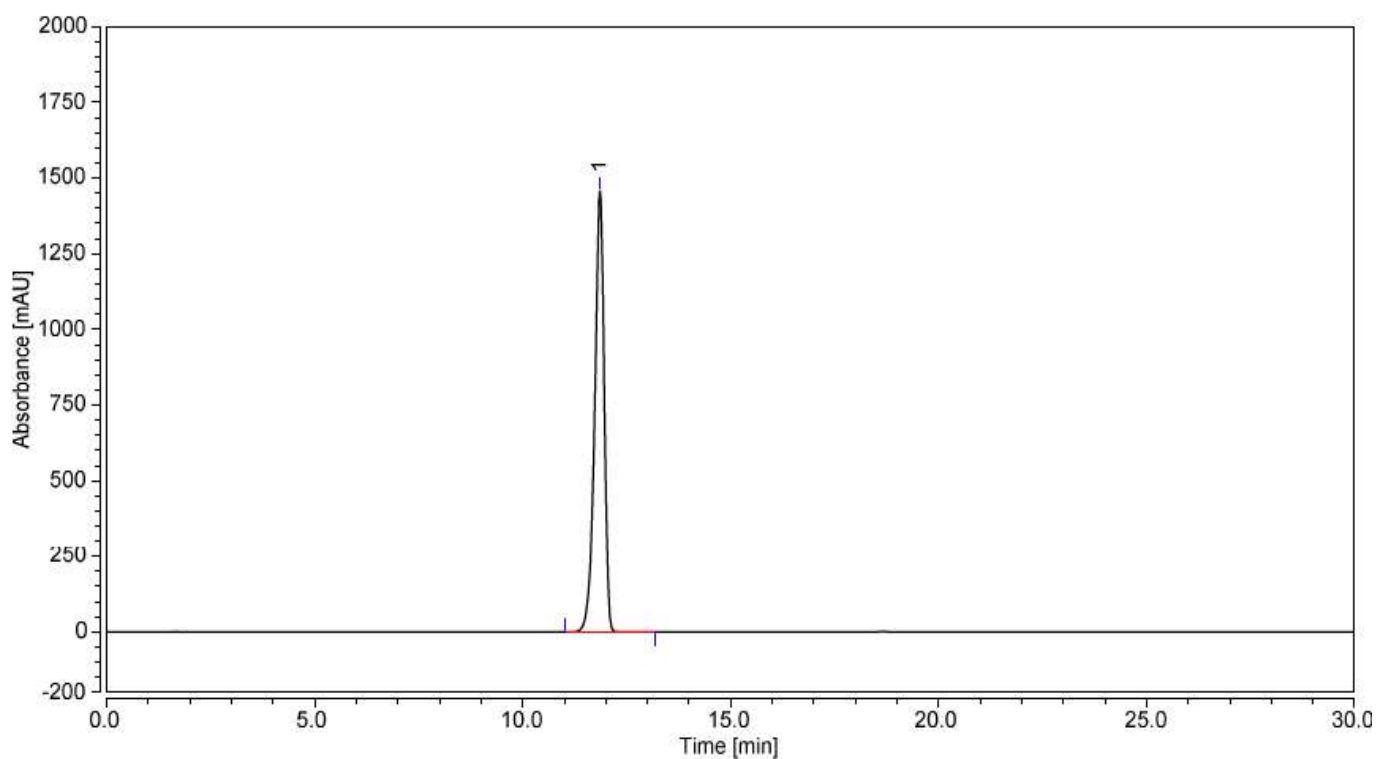

1. Bosentan (USP assay)

HPLC condition

Column	INNO Column Phenyl (5um, 4.6mm I.d. × 250mm)
	Buffer / ACN = 55 / 45
Mobile Phase	Buffer : Mix 1mL of triethylamine with 1L of water. Adjust with phosphoric acid to a pH of 2.5.
Flow rate	1.5mL/min
Temperature	35℃
Detector	UV (220nm)