


# HPLC DATA SHEET

## Buspirone HCl Tablets(USP, Assay)

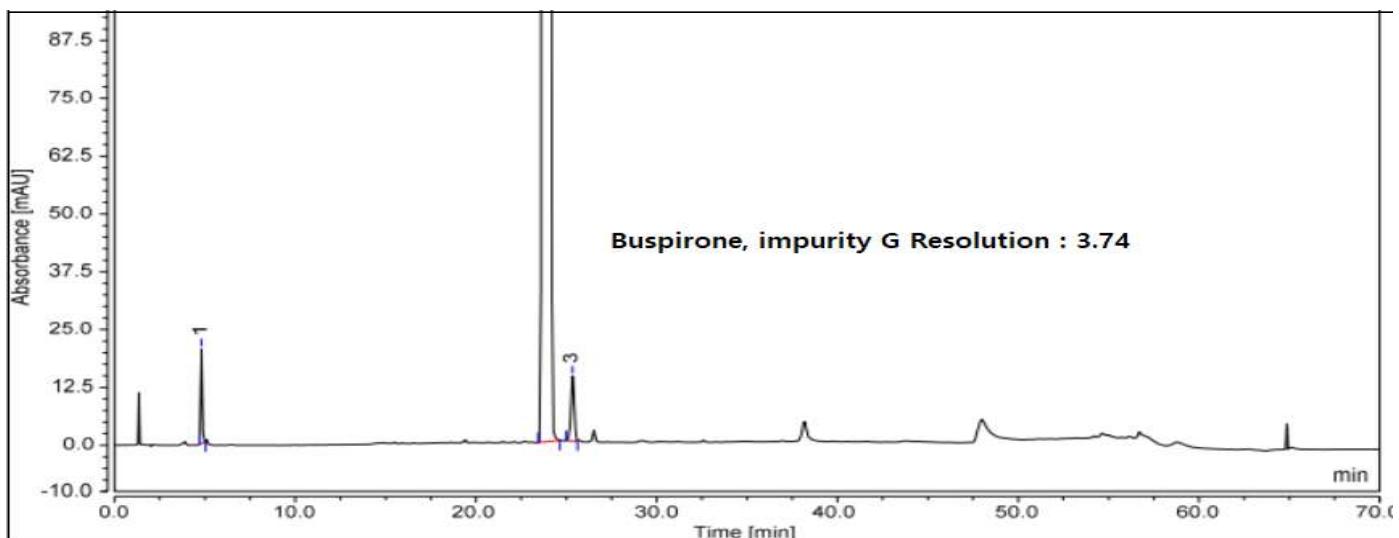

1. Impurity A    2. Buspirone    3. Impurity G

### HPLC condition

Column	INNO Column C18-HC (5um, 4.6mm I.d. × 150mm) Mobile phase A : Acetonitrile : Solution A (5 : 95) Mobile phase B : Acetonitrile : Solution B (75 : 25) *Solution A : Dissolve 6.8g of Potassium dihydrogen phosphate and 0.93 g of 1-Hexanesulfonic acid sodium salt in water to make 1000 mL. (adjust the pH to 3.4 with phosphoric acid) *Solution B : Dissolve 3.4g of Potassium dihydrogen phosphate and 3.52 g of 1-Hexanesulfonic acid sodium salt in water to make 1000 mL. (adjust the pH to 2.2 with phosphoric acid)																											
Mobile Phase	<Gradient System>																											
	<table border="1"><thead><tr><th>min</th><th>A(%)</th><th>B(%)</th></tr></thead><tbody><tr><td>0</td><td>90</td><td>10</td></tr><tr><td>6</td><td>90</td><td>10</td></tr><tr><td>34</td><td>42</td><td>58</td></tr><tr><td>45</td><td>42</td><td>58</td></tr><tr><td>55</td><td>0</td><td>100</td></tr><tr><td>56</td><td>100</td><td>0</td></tr><tr><td>60</td><td>100</td><td>0</td></tr><tr><td>61</td><td>90</td><td>10</td></tr></tbody></table>	min	A(%)	B(%)	0	90	10	6	90	10	34	42	58	45	42	58	55	0	100	56	100	0	60	100	0	61	90	10
min	A(%)	B(%)																										
0	90	10																										
6	90	10																										
34	42	58																										
45	42	58																										
55	0	100																										
56	100	0																										
60	100	0																										
61	90	10																										
Flow rate	1.0mL/min																											
Temperature	40°C																											
Injection Vol.	20uL																											
Detector	UV (240nm)																											