


HPLC DATA SHEET

Betadex (USP, Assay)

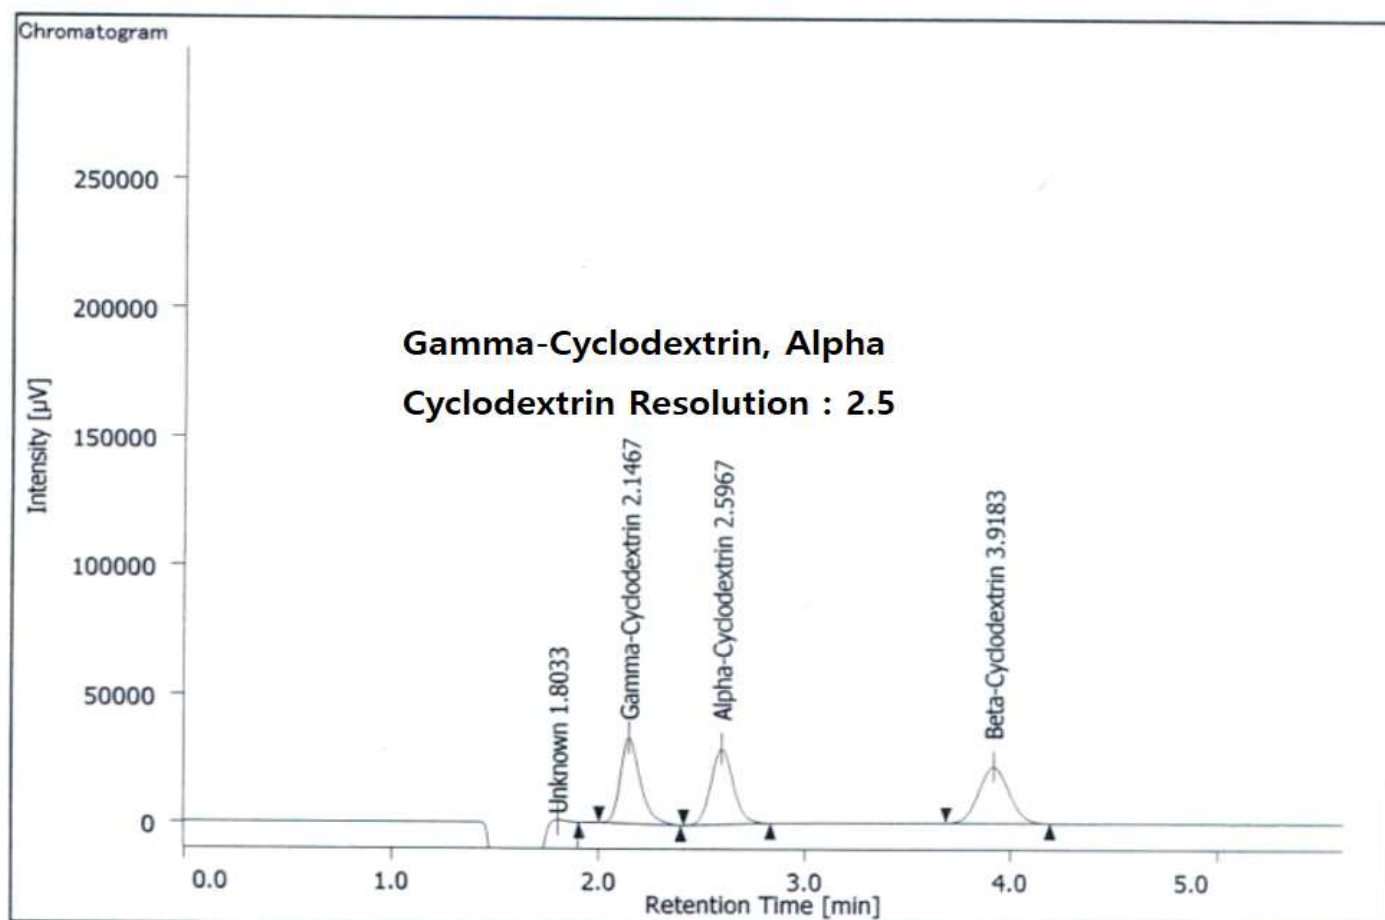

1. Gamma-Cyclodextrin 2. Alpha-Cyclodextrin 3. Beta-Cyclodextrin

HPLC condition

Column INNO-P Column C18 (5µm, 4.6mm I.d. × 150mm)

Mobile Phase Methanol : Water = (7 : 93)

Flow rate 1.5mL/min

Temperature Column : 30°C
Detector : 40°C

Detector RI

Injection Vol. 50µL